




खडक नगरपालिका  
नगर कार्यपालिकाको कार्यालय

०३१-५४००५४




पत्र संख्या:-२०८२/०८३

चलानी नं.: १२१६

मिति: २०८२/१२/२६

**विषय:- सर्जिकल सामग्री र अस्पतालको औजार एवम उपकरणहरूको लागत ईस्टिमेट प्रयोजनका लागि दररेट पेश गर्ने बारे।**

प्रस्तुत विषयमा यस खडक नगरपालिका वडा नं ०७ मा अवस्थित आधारभूत अस्पताल कल्याणपुर, सप्तरी संचालनका लागि सर्जिकल सामग्री र अस्पतालको औजार एवम उपकरणहरू खरिद गर्न लागत ईस्टिमेट प्रयोजनका लागि यसै पत्र साथ संलग्न प्रमाणित सूची बमोजिम आवश्यक सामग्रीहरूको दररेट सार्वजनिक खरिद नियमावली ऐन, २०६३ तथा खरिद नियमावली २०६४ को १४ औं संशोधन २०८२ को अधिनमा रही नियम पूर्वक सरसामानहरूको यस कार्यालयबाट प्रमाणीत सूचीमा उल्लेखित स्पेशिफिकेशन अनुसार फर्म ईजाजत तथा आ.व २०८२/०८३ को नविकरण भएको प्रमाणपत्र, मु.अ.कर, दर्ता प्रमाणपत्र र २०८२/०८३ को कर चुक्ता प्रमाणपत्र समेत राखि मु.अ.कर बाहेकको दररेट ७ दिन भित्र पेश गर्नुहुन अनुरोध छ ।

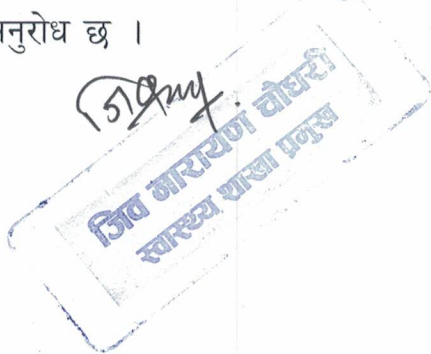

हरेन्द्र कुमार श्रेष्ठ

प्रमुख प्रशासकीय अधिकृत


हरेन्द्र कुमार श्रेष्ठ


प्रमुख प्रशासकीय अधिकृत



आधारभूत अस्पताल कल्याणपुर,सप्तरीको लागि सर्जिकल सामग्री र अस्पताल औजार एवमं उपकरणहरूको दररेट माग विवरण


सि.न	सरसामानहरूको नाम	स्पेसिफिकेसन	संख्या	दररेट		कैफियत
				अक	अक्षर	
1	Medicine Trolley	<ul style="list-style-type: none"> <li>• Frame work made of stainless steel tubular pipe mounted on four castors.</li> <li>• Two fixed S.S. shelves of heavy gauge with three side railing.</li> <li>• ISO/CE certified.</li> </ul>				
2	Suction Machine	<p>Powder coated body fitted with S.S top Heavy Duty motorized pump for fast vacuum built - up. Noiseless. Finely regulable 0-700mm Hg or more vacuum.</p> <p>Over Flow Safety Device: over - flow check valve and removable filter to protect</p> <p>Max Vacuum: - 700 or more mm Hg regulable through Vacuum Control Knob. ISO/CE certified.</p>				
3	Needle Destroyer Pics	<ul style="list-style-type: none"> <li>• Versatility: Features 3-in-1 operation capabilities in a single compact body - electric burning of needles, cutting of syringes, and a manual cutting option for use during power outages.</li> <li>• Durability: Constructed with a strong metal body and powder-coated for enhanced longevity and resistance to wear and tear.</li> </ul>				

  
**जिव नारायण चौधरी**  
 स्वास्थ्य शाखा प्रमुख

  
**हरेन्द्र कुमार श्रेष्ठ**  
 प्रमुख प्रशासकीय अधिकृत

		<ul style="list-style-type: none"> <li>• Power Requirements: Operates on AC 220V - 50Hz, making it compatible with standard electrical supplies.</li> <li>• ISO/CE certified.</li> </ul>			
4	Drum (Small Pics)	<ul style="list-style-type: none"> <li>• Multiple Size Options: Includes large-capacity models – Approx. 15x12, 11x9, 9x9, and 8x6 inches – for varied medical needs.</li> <li>• Crystal Mirror Polish Finish: Easy-to-clean, hygienic surface with a professional-grade appearance.</li> <li>• Corrosion-Resistant &amp; Autoclavable: Reusable design withstands repeated high-temperature sterilization cycles.</li> <li>• Secure Lock &amp; Ventilation Slots: Ensures tight closure and optimal steam circulation for effective sterilization.</li> <li>• Durable &amp; Reusable: Built with strong welds and double-reinforced edges for extended life and maximum load capacity.</li> </ul>			
5	Intubation Set Pics	<p>Laryngoscope Handle: reusable and chrome-plated, with fiber optic (F.O.) technology.</p> <p>Laryngoscope Blades: includes multiple sizes of Macintosh (curved) or Miller (straight) blades, ranging from 0 (infant) to 4 (adult).</p> <p>Endotracheal (ET) Tubes: Cuffed tubes (ranging from sizes 5.0 mm to 10.0 mm) or uncuffed tubes for pediatric use (sizes Approx. 2.5 mm - 4.0 mm).</p> <p>Intubating Stylet: Used to stiffen the ET tube and provide shape.</p> <p>Magill Forceps: Used to guide the tube, particularly in nasal intubation.</p> <p>Guedel Airways: Oropharyngeal airways, often in sizes 0-4.</p> <p>Syringe: A 10 mL syringe for inflating the cuff of the ET tube.</p> <p>Lubricant: Sterile, water-soluble jelly.</p>			

13/10/2023

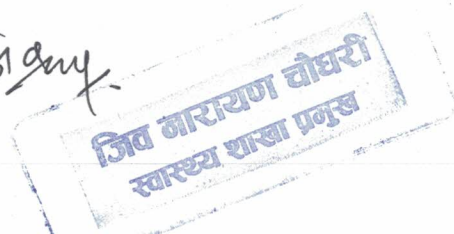

हरेन्द्र कुमार श्रेष्ठ  
प्रमुख प्रशासकीय अधिकृत

		Fixation Device: Tape or tube holder to secure the tube.			
6	Pulse Oxymeter Pics	Technology - Non-invasive measurement of the arterial oxygen saturation (SpO2) and the heart rate (pulse rate) on the finger Accuracy - 70 - 100% , Pulse 30-200 or more bpm. Measurement range - SpO2 0 - 100%, pulse 0 - 250 or more heart beats ISO/CE certified.			
7	Suturing Set	<ul style="list-style-type: none"> <li>The set of 5 Pcs contains - Needle Holder, Dissecting Forceps Tooth, Heath Suture Scissors, Scalpel Handle. Mosquito Artery Forceps Cvd ,</li> <li>Made from surgical grade steel</li> <li>Corrosion free stainless steel</li> <li>ISO and CE certified.</li> </ul>			
8	Suture Set/Suture Out Set	<ul style="list-style-type: none"> <li>- Kidney Dish - medium</li> <li>- Gallipot - medium</li> <li>- Mayo Hegar needle holder</li> <li>- Dressing Forceps (Thumb)</li> <li>- English TOE dissecting forceps - plain</li> <li>- Dissecting forceps toothed 1x2</li> <li>- Suture scissors - Heaths Ligature</li> <li>- Mayo scissors - straight.</li> </ul>			
9	Epistomy Set	Ramplie Sponge Holding Forceps Braun Stadler Episiotomy Scissors Gillies Tissue Forceps. Mayo Hegar Dental Syringe Op-scissors sh/bl str.			
10	Dressing Trolley	Material: AISI 304 Stainless Steel (Grade 304 is standard for corrosion resistance and easy cleaning). Dimensions: Average dimensions are Approx.700-750 mm length/width and 800-900 mm height. Shelves: Two to three stainless steel shelves, often featuring raised edges (safety railings) to prevent equipment from falling.			

डिप्टी  
जिव नारायण चौधरी  
स्वास्थ्य शाखा प्रमुख

नगर  
महिला का कौशल  
केल्याणपुर, सप्तरी  
मधेश प्रदेश, नेपाल  
१९३

६९ हरेन्द्र कुमार श्रेष्ठ  
प्रमुख प्रशासकीय अधिकृत

		Castors: Four castor wheels, usually 75 mm to 100 mm in diameter, with at least two equipped with brakes for stability, frequently including anti-static features. ISO/CE certified.			
11	Delivery Set	<ul style="list-style-type: none"> <li>• Sterilization: Methods and protocols for ensuring all instruments are sterile and ready for use.</li> <li>• Material Quality: Requirements for medical-grade materials, often stainless steel, ensuring durability, corrosion resistance, and autoclavability.</li> <li>• ISO/CE certified.</li> </ul>			
12	Emergency Trolley Crash Cart	<p>Complete S.S. 304 Grade Tubular Work with Top with Three Sided Stainless Steel Railing 304 Grade</p> <p>Trolley Mounted on 125mm Dia Castor Two with Brakes and Two without Brakes.</p> <p>Six Molded Drawers, two Drawers with Utility Containers</p> <p>handout Bins at Eye Level</p> <p>S.S. Saline Rod and Detachable Powder Coated Oxygen Arrangement</p> <p>One Wooden Board for Cardiac Massage</p> <p>Complete S.S. in Matte Polish Finish</p>			
13	Perineal Vaginal Cervical Repair Set	<p>Retractors: speculum (posterior) and right-angled vaginal retractors (anterior/lateral) to ensure clear visualization of the cervix.</p> <p>Forceps Ring forceps (Sponge Sticks) are critical for grasping the friable cervical tissue without causing further damage.</p> <p>Forceps (Toothed/Long): Long forceps (smooth and toothed, 10-inch) to hold tissue securely, such as Teale vulsellum forceps or single-tooth tenaculum.</p> <p>Needle Holder: Long, heavy-duty needle holder.</p> <p>Scissors: Long, curved, or straight Mayo scissors.</p>			

13/9/24  
 जित नारायण चौधरी  
 स्वास्थ्य शाखा प्रमुख

खडक नगरपालिका कार्यलय  
 नगर कार्यपालिकाको कार्यालय  
 कल्याणपुर, सप्तरी  
 मधेश प्रदेश, नेपाल  
 २०७३

हरिन्द्र कुमार श्रेष्ठ  
 प्रमुख प्रशासकीय अधिकृत

		Sutures: Absorbable, synthetic materials often with a 3/8 or 1/2 circle, tapered or round-point needle, 30-50 mm length.			
14	Defibrillator Aed	Waveform: Biphasic Truncated Exponential (BTE) or Rectilinear Biphasic. Energy Selection: 50J-200J or more (adult). Charging Time: Generally <10 seconds to 200 Joules. Self-Tests: Daily, weekly, or monthly automatic self-tests. ISO/CE or USFDA approved.			
15	Chetal Forcefs	• High-Quality Material: Made from premium, corrosion-resistant stainless steel for durability and longevity.			
		Glass - 6mm Tempered or better.  Weighing Capacity - 180 kg or more			
16	Weight Machine Adult Peadiatric	Accuracy - 100 g or better  Display - LCD Screen Display With Black Backlight And White Digits.			
17	Fetal Dopler	• Ultrasonic Frequency: 2.5 MHz or better • Continuous work time: 7 hours or more • ISO/CE certified.			
18	Dressing Trolly	Material: High-quality Stainless Steel, offering corrosion resistance, durability, and easy cleaning.			
		• The syringe-driver can be used with following volume syringes: 10 ml, 20 ml, 30 / 35 ml and 50 ml. • Display range of volume delivered: 0.1 to 999 ml or more. • Occlusion detection pressure :			

Signature

जित नारायण चौधरी  
स्वास्थ्य शाखा प्रमुख

खडक नगरपालिका  
नगर कार्यपालिकाको कार्यालय  
कल्याणपुर, सप्तरी  
मधेश प्रदेश, नेपाल  
२०७३

हरेन्द्र कुमार श्रेष्ठ  
प्रमुख प्रशासकीय अधिकृत

19	Syringe Pump	<p>High (H) : 800 mmHg +/- 200 mmHg  Center (C) : 500 mmHg +/- 100 mmHg  Low (L) : 300 mmHg +/- 100 mmHg</p> <ul style="list-style-type: none"> <li>• Power voltage : AC 110 V - 230 V</li> <li>• Backup: more than 6 hours at a speed of 5 ml/hour.</li> </ul>				
20	Infusion Pump	<ul style="list-style-type: none"> <li>• ISO/CE certified.</li> <li>• Manual/Automatic Bolus</li> <li>• Vertical &amp; Horizontal mounting clamp.</li> <li>• Anti-bolus system.</li> <li>• DPS dynamic pressure display.</li> <li>• 1000 or more events stored can be checked and downloaded</li> <li>• Large color TFT display with adjustable brightness.</li> <li>• ISO /CE certified.</li> </ul>				
21	Digital Thermometer	<ul style="list-style-type: none"> <li>• accuracy and fast response</li> <li>• Last reading memory display.</li> <li>• Beep alarm when peak temperature is reached.</li> <li>• Auto shut-off function.</li> <li>• Without mercury, suitable for use at home and hospitals.</li> <li>• Provides quick and highly accurate body temperature reading.</li> <li>• With beep alarm and memory function.</li> <li>• ISO/CE certified.</li> </ul>				
22	Ctg Machine	<ul style="list-style-type: none"> <li>• 8" or more colorized LCD large Screen</li> <li>• Long life-span recorder with array of high heat, print immediately or After storing</li> <li>• Double event marks</li> <li>• Three-in-one probe, reduce the line winding.</li> <li>• Code-operation, easy and convenient</li> <li>• A variety of alarming functions</li> <li>• Automatic fetal movements function</li> </ul>				

Signature

जित नारायण चौधरी  
स्वास्थ्य शाखा प्रमुख

हरेंद्र कुमार श्रेष्ठ  
प्रमुख प्रशासकीय अधिकृत



